

ISOVP PROBE QUICK REFERENCE GUIDE

TURNING ON

TURNING ON THE RECEIVER

TURNING ON THE PROBE HEAD

SHORTLY PRESS
TURN ON
BUTTON

SHORTLY PRESS
TURN ON
BUTTON

RECEIVER
TURNS ON

PROBE
TURNS ON

LOW POWER MODE

GOING INTO LOW POWER MODE

EXITING LOW POWER MODE

SHORTLY PRESS
TURN ON
BUTTON IN
EITHER UNIT

SHORTLY PRESS
TURN ON
BUTTON IN
EITHER UNIT

UNITS IN STDBY:
ON LED BLINKS
IN BOTH UNITS


UNITS IN
NORMAL MODE:
LED ON IN BOTH
UNITS

PROBE CALIBRATION

CAL LED STATE: CALIBRATION 

SHORT BLINK EVERY 3 SECS: CAL REQUIRED
LONG BLINK EVERY 3 SECS: CAL ERROR

TEST AND CALIBRATION

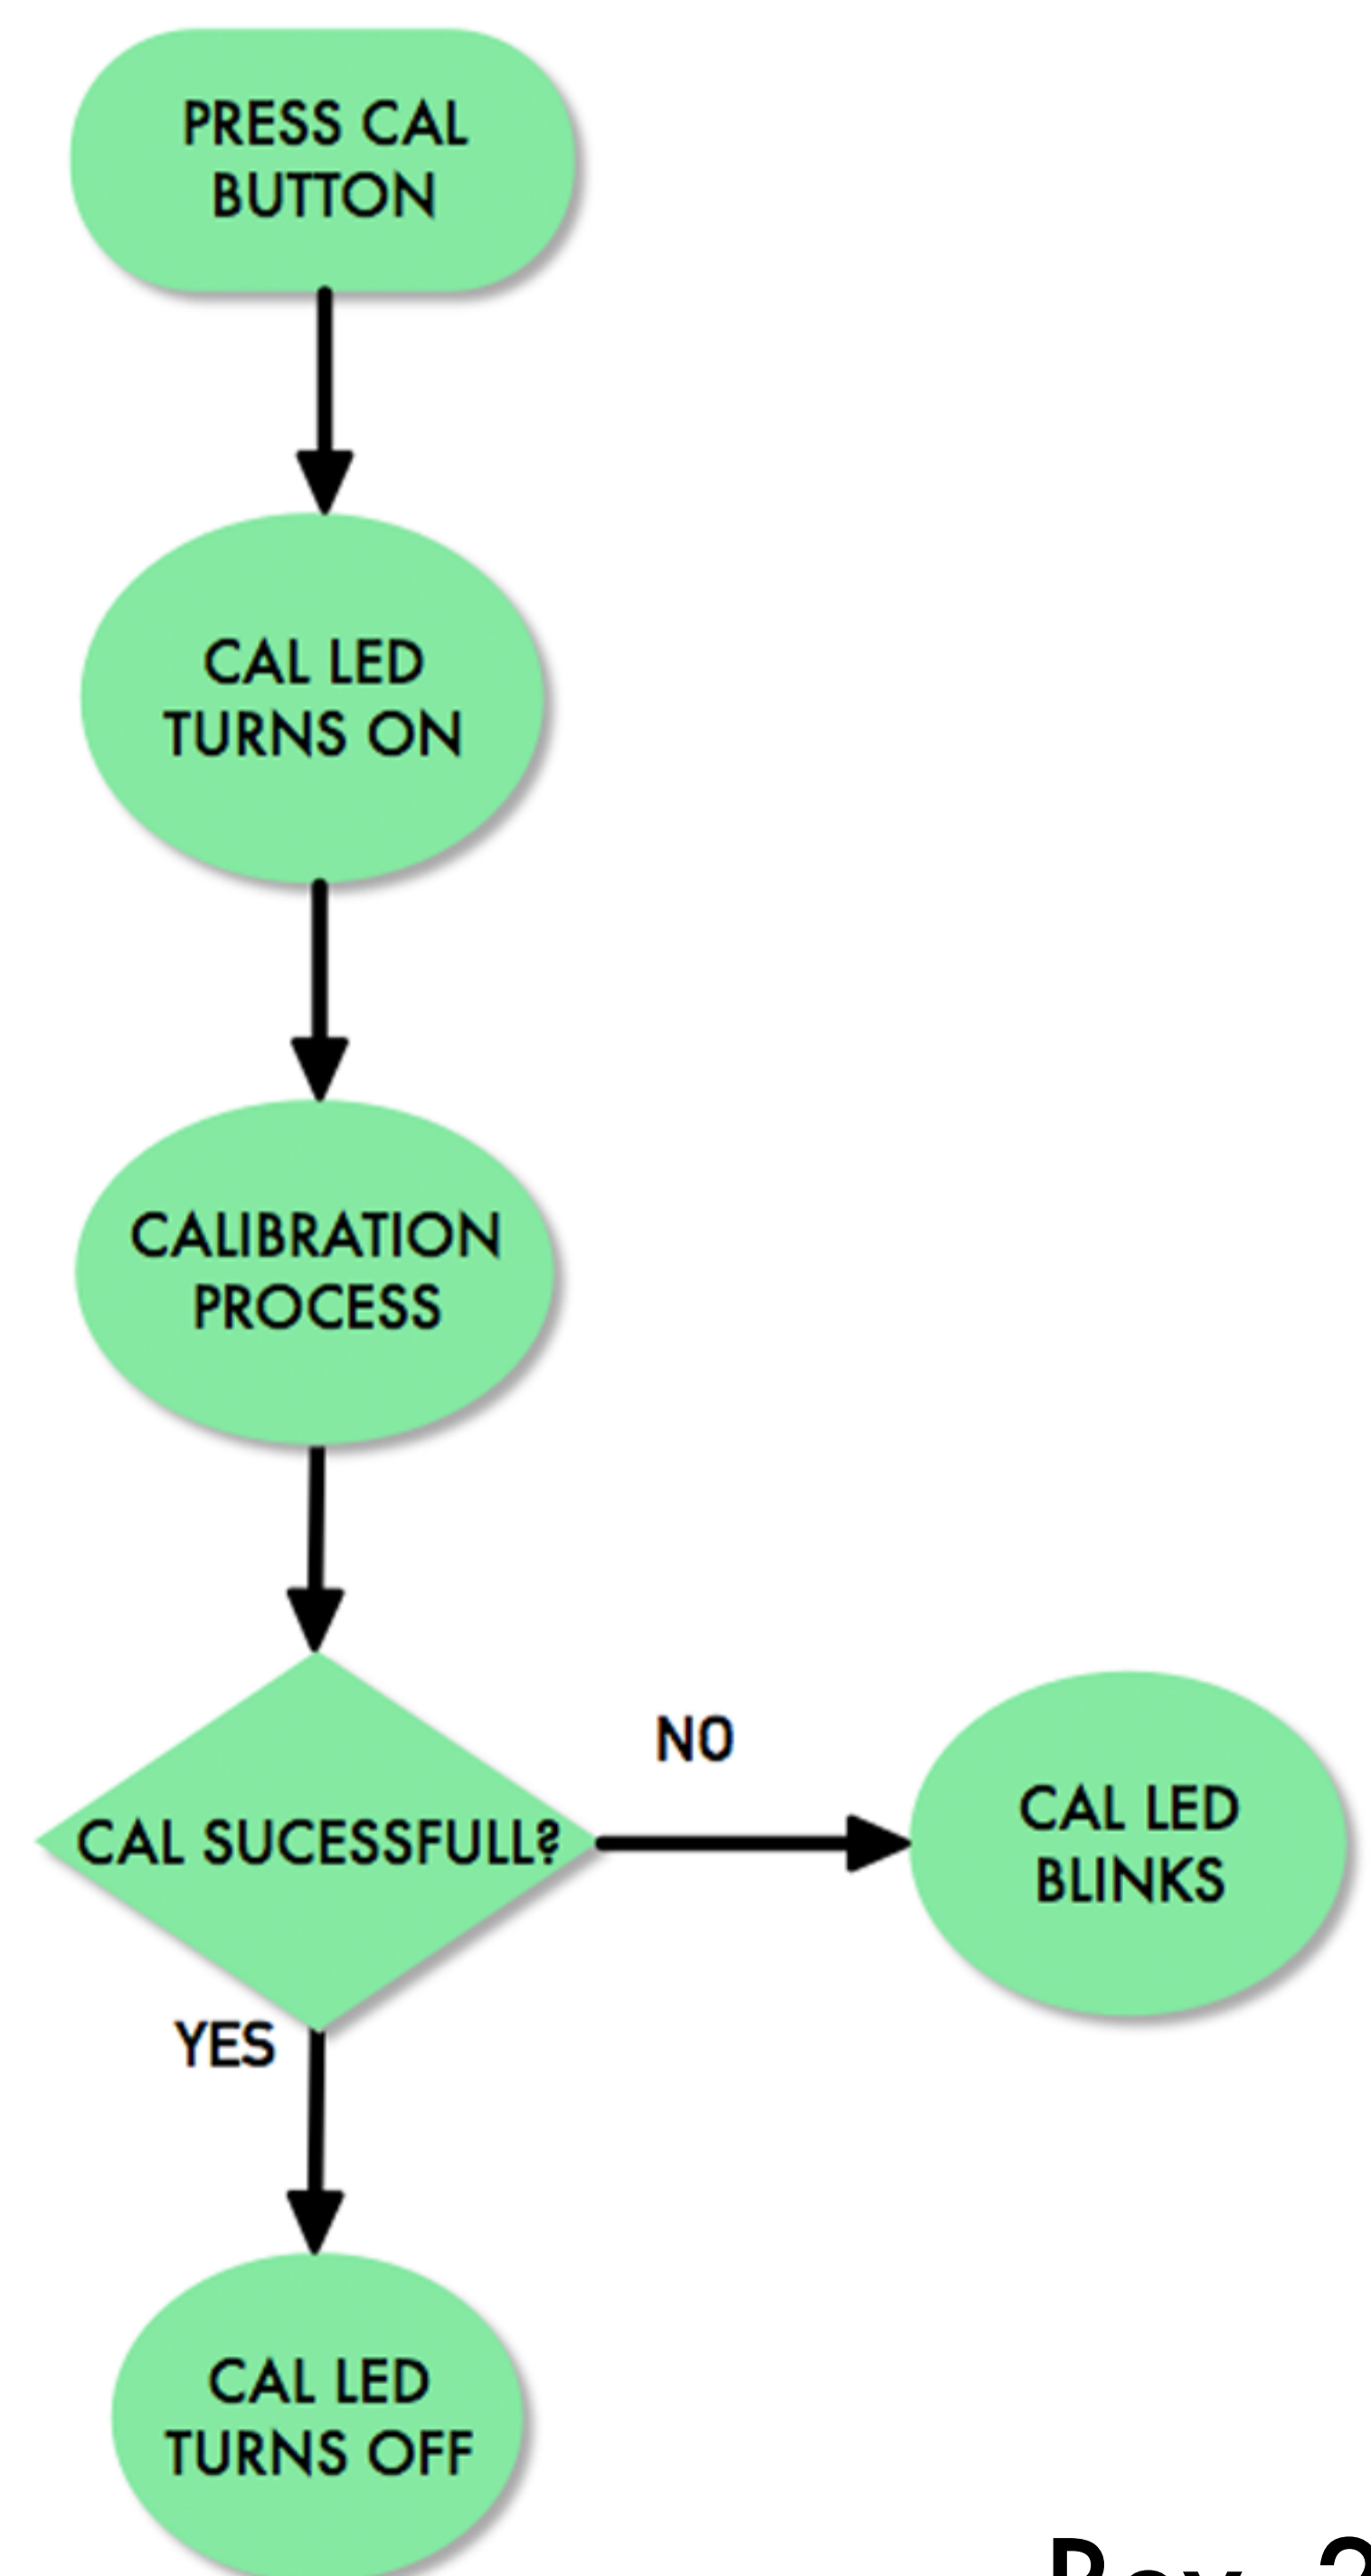

TURNING OFF

TURNING OFF PROBE HEAD
AND RECEIVER

PRESS TURN
ON BUTTON
1 sec IN
EITHER UNIT

BOTH UNITS
TURNS OFF

LOW BATTERY LED

INDICATES TX BATTERY LOW STATUS

BATT LOW 

- ▶ ALWAYS CONNECT RECEIVER TO A 50 Ohm TERMINATED SCOPE
- ▶ DO NOT PULL OR BEND THE FIBER CABLES AT SHARP ANGLES

**DO NOT USE THE PROBE HEAD OR ITS ACCESORIES FOR
HANDHELD MEASUREMENTS**